


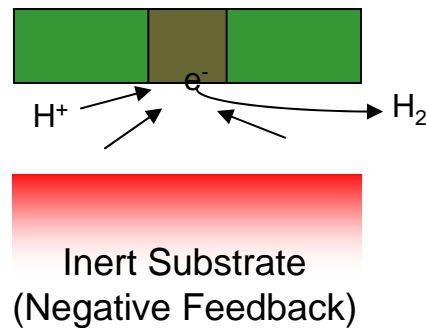



# SECM Approach Curves



- Bias tip so that proton reduction occurs spontaneously.
- Bias substrate so that hydrogen oxidation reaction occurs at catalyst sites.
- Move tip and monitor current to find active sites.

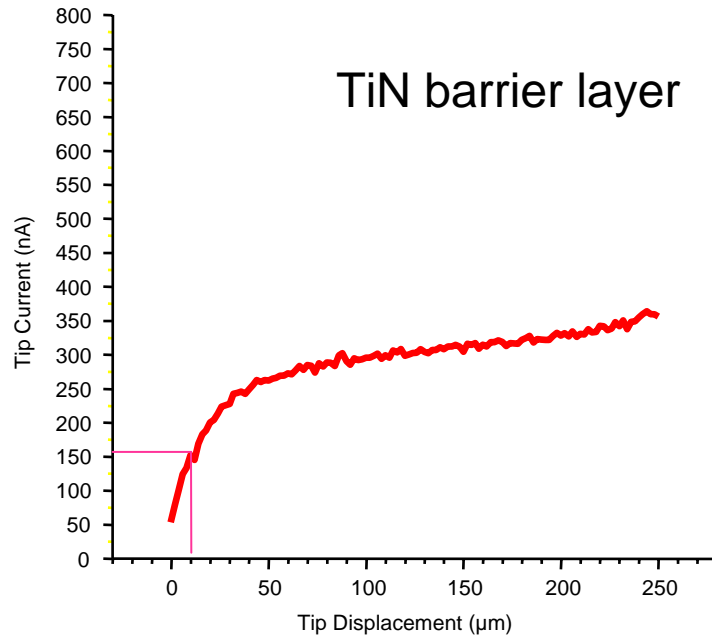